



(11) **EP 3 082 631 B1**

(12) **EUROPEAN PATENT SPECIFICATION**

(45) Date of publication and mention of the grant of the patent:
16.10.2019 Bulletin 2019/42

(21) Application number: **14805935.5**

(22) Date of filing: **03.12.2014**

(51) Int Cl.:
A61B 17/72 (2006.01) A61B 17/86 (2006.01)

(86) International application number:
PCT/EP2014/076340

(87) International publication number:
WO 2015/090954 (25.06.2015 Gazette 2015/25)

(54) **INTRAMEDULLARY DEVICE FOR MID-SHAFT CLAVICLE FRACTURES**

INTRAMEDULLÄRE VORRICHTUNG FÜR MITTEL-KLAVIKULA-SCHAFTFRAKTUREN

DISPOSITIF INTRAMÉDULLAIRE POUR FRACTURE MÉDIODIAPHYSAIRE DE LA CLAVICULE

(84) Designated Contracting States:
AL AT BE BG CH CY CZ DE DK EE ES FI FR GB GR HR HU IE IS IT LI LT LU LV MC MK MT NL NO PL PT RO RS SE SI SK SM TR

(30) Priority: **17.12.2013 EP 13197625**

(43) Date of publication of application:
26.10.2016 Bulletin 2016/43

(73) Proprietor: **Stichting Katholieke Universiteit 6525 EZ Nijmegen (NL)**

(72) Inventor: **HOOGERVORST, Paul 6525 EZ Nijmegen (NL)**

(74) Representative: **Nederlandsch Octrooibureau P.O. Box 29720 2502 LS The Hague (NL)**

(56) References cited:
DE-A1- 3 924 610 US-A- 4 640 271
US-A- 5 374 235 US-A1- 2009 306 718

EP 3 082 631 B1

Note: Within nine months of the publication of the mention of the grant of the European patent in the European Patent Bulletin, any person may give notice to the European Patent Office of opposition to that patent, in accordance with the Implementing Regulations. Notice of opposition shall not be deemed to have been filed until the opposition fee has been paid. (Art. 99(1) European Patent Convention).

Description

Field of the invention

[0001] The present invention relates to an intramedullary device for treatment of a fracture of a long pipe bone, such as a (mid-shaft) clavicle fracture.

Prior art

[0002] US patent US 4,640,271 (Lower) discloses a bone screw having a main shaft and a separate sleeve member. The main shaft has a first set of threads on a leading end portion and an elongated smooth unthreaded shaft portion with a protruding lip on the opposite, trailing end of the main shaft. The separate sleeve member, provided with a second set of threads on its outer surface, is held in position by the protruding lip on the unthreaded shaft portion, but only in one direction. No axial stability is provided by the bone screw, and also no flexibility is provided.

[0003] US patent publication US 2009/306718 discloses a lagwire system for facilitating fixation of bone fractures. An anchor component is provided as well as a wire, a threaded sleeve, a tubular sleeve and a cap. The lagwire system is only suitable for exerting a compressing force, and no rotation at the fixation position is possible.

[0004] US patent 6,338,732 discloses an in marrow nail structure having a pin with two threaded ends. Lateral fixation is accomplished outside of the fractured bone. After fixation of the in marrow nail structure, no rotation is possible anymore, and also no axial stability is provided.

[0005] American patent publication US2011/0009865 discloses an intramedullary pin for bone fixation in a clavicle fracture. At one end, the pin is fastened using a screw threaded part, and at the other side of the fracture, the pin is fixated using a fastener in a transverse aperture in the pin.

[0006] International patent publication WO2011/060412 discloses a pre-curved intramedullary clavicle nail, which can be anchored to the bone using one or two fixation elements, such as screws.

[0007] US-A-5,374,235 discloses a marrow nail with a plurality of screws for securing the nail in a bone of a patient. The marrow nail includes a plurality of recesses defined proximate one end of an elongated rod. Each of the plural recesses is formed as a notch and is operably engageable with a respective one of the plural screws.

Summary of the invention

[0008] The present invention seeks to provide an improved intramedullary device especially suited for treatment of a fracture of a long pipe bone, such as a (mid-shaft) clavicle fracture.

[0009] According to the present invention, an intramedullary device according to claim 1 is provided.

[0010] Due to the components of the present invention intramedullary device embodiments, once in place the connection between the two fractured clavicle parts will be rigid in the axial plane so it will prevent the mid-shaft clavicle fracture from shortening but remains free to rotate within itself to prevent hardware failure and implant migration. The surgical technique needed for implantation of the present device embodiments is minimally invasive. It is expected that time needed for the procedure is shorter and less invasive than by using the current standard therefore being more cost effective and cheaper as well.

Short description of drawings

[0011] The present invention will be discussed in more detail below, using a number of exemplary embodiments, with reference to the attached drawings, in which

Fig. 1 shows a side view of a base pin of an embodiment of the intramedullary device according to the present invention;

Fig. 2 shows an enlarged sectional side view of a connection part of the base pin of Fig. 1, which allows selection of an appropriate length of the intramedullary device;

Fig. 3a and 3b show a side view and a cross sectional view of a secondary fixation element as part of an embodiment of the intramedullary device according to the present invention;

Fig. 4a and 4b show a perspective view and a cross sectional view of an end cap to be used in conjunction with the secondary fixation element of Fig. 3a and 3b;

Fig. 5 shows a perspective view of a first tool to be used with the intramedullary device according to the present invention embodiments; and

Fig. 6 shows a perspective view of a second tool to be used with the intramedullary device according to the present invention embodiments.

Detailed description of exemplary embodiments

[0012] The present invention provides a number of embodiments of an intramedullary (fixation) device for mid shaft clavicle fractures (MSCF) as specific application, and more general for treatment of a fracture of a long pipe bone. Currently available intramedullary implants do not have the properties for optimal reduction and conservation of the anatomical shape and length of the clavicle when fractured. The proposed solution embodiments provide a device that is able to re-establish anatomical alignment, prevent shortening and is able to rotate freely within itself, all in a minimally invasive manner. It is expected that time needed for the procedure is shorter, the implants are cheaper, rehabilitation will be similar and therefore will be more cost-effective than by using the current standard or other minimally invasive devices.

[0013] Clavicle fractures approximately constitute for

5% of all fractures. About 69-82% of these fractures are mid-shaft clavicle fractures (MSCF). Because of the specific s-shaped anatomy and muscle insertions, about 73% of these fractures are displaced and/or shortened. These two features have been found to be poor predictors of outcome concerning non-unions, persistent posttraumatic symptoms and cosmetics in conservatively treated MSCF. Therefore, lately the tendency has been to surgically reduce and fixate MSCF if shortened more than 2cm or displaced more than the diameter of the clavicle's shaft. The standard for these operations now is fixation using a (angle-stable) plate and screws. This method creates a rigid fixation of both fracture elements and aims for primary bone healing. It re-establishes the normal length and alignment of the clavicle. Patients are able to quickly start rehabilitating. There have been reports that operative interventions results in better rates of union, less mal-unions and increased patient satisfaction. The downsides of these procedures are a large incision and scarring, risk of infection, and need for hardware removal in about half of the patients because of irritation.

[0014] Another frequently used technique to reduce and align MSCF is by using intramedullary devices. Examples of these devices are straight rigid pins (Hagie, Knowles, Rockwood) and titanium elastic nails (TEN). The first one aims for primary bone-healing and requires an inside-out open reduction operative technique which means loss of the fracture hematoma. It has produced contradictory results. The latter aims for secondary fracture healing by not evacuating the fracture hematoma with all its bone-healing substances. TEN is minimally invasive; it requires smaller incisions. Also hardware removal if necessary is easier and less invasive. Because of the flexibility of TEN it allows itself to follow the shape of the clavicle and re-align the MSCF. Good results have been reported using TEN. The downside of TEN is that they do not protect the MSCF from shortening and subsequent forming of a possible symptomatic malunion. Other negative features of TEN are well documented implant migration because it is not fixated well within the clavicle and a high rate of implant removal after healing of the fracture has occurred.

[0015] To create an optimal method of fixating MSCF all of the issues described above need to be taken into account. The device would need specific features. It should be intramedullary so it is less invasive. An intramedullary device would also make it possible to prevent evacuation of the fracture hematoma so secondary bone-healing can be pursued. It should be flexible enough to follow the s-shaped contour of the clavicle. It has to be rigid enough to be able to re-align and prevent shortening of the MSCF. It should be fixated in both fracture elements to prevent shortening and migration. It must be simple to implant and simple to remove if necessary. If these requirements are met it is likely that this device will be superior to the current standard of plate osteosynthesis.

[0016] According to the present invention embodi-

ments an intramedullary device for treatment of fracture of a long pipe bone (such as a mid-shaft clavicle fracture) is provided, comprising a (flexible or at least bendable) base pin 1 having a primary fixation element 2 and a connection part 3, and a secondary fixation element 6 attachable to the connection part 3 at one of a plurality of predetermined distances along the base pin with respect to the primary fixation element 2. The connection part 3 of the base pin 1 and the secondary fixation element 6 are rotatable (or rotationally free) with respect to each other when attached. The axial position of the secondary fixation element 6 with respect to the primary fixation element 2 is then fixed. This means axial stability in which the length of the base pin 1 (and the clavicle) cannot change in any of the two axial directions while at the same time the freedom to rotate within itself (i.e. locally where the secondary fixation element 6 is attached) will prevent hardware failure and subsequent implant migration and/or shortening of the (implanted) intramedullary device.

[0017] An embodiment of such an intramedullary device is shown as parts depicted in Fig 1-4b as will be described below. Fig. 1 shows a side view of an embodiment of a base pin 1, having a total length of $l_1+l_2+l_3+l_4$ as shown. The (flexible) base-pin 1 can easily be implanted intramedullary through the clavicle's two fracture elements so alignment is obtained. The base pin 1 has a primary fixation element 2, which in the embodiment shown comprises a self-tapping threaded head end (2a), allowing fixation of the base pin in a sternal or medial end of the clavicle. By using a threaded head end 2a implantation will be more controlled and thus safer than by using TEN. The self-tapping threaded head end (2a) is provided with a blunt tip part (2b), to prevent perforation into the sterno-clavicular joint. The tip 2b is e.g. provided with a radius of 12.7mm over 90°, when the main diameter of the base pin 1 is e.g. 2 mm. The threaded head-end 2a is provided with a screw thread having a pitch distance which is adapted for its use in anchoring the base pin 1 in the clavicle.

[0018] As shown in the embodiment of Fig. 1, the base pin 1 further comprises a handling part 4 remote from the primary fixation element 2. A special tool can e.g. be attached to this handling part 4, e.g. allowing exertion of a screwing motion to fix the primary fixation element 2 inside the clavicle bone.

[0019] In order to cater for the internal shape of the clavicle bone, the base pin 1 is bendable in a further embodiment. This can e.g. be accomplished by selecting the right material, e.g. stiff yet bendable such as AISI 304 stainless steel, in combination with a proper diameter (e.g. 2 mm). Alternatively, the base pin 1 is made of another medical grade material, such as titanium.

[0020] The secondary fixation element 6, or intra-cortical fixation device, is positioned in the dorsolateral aspect of the clavicle in use near the conoid process to allow fixation within the bone and around the base pin 1 at the appropriate length. Eventually, the base pin 1 will

be cut at the appropriate length. An end cap or locking screw 7 (see below for further details thereof) may fixate the secondary fixation element 6 to the connection part 3 at the correct length and on both sides of the fractures.

[0021] As shown in the embodiment of Fig. 1, the connection part 3 is provided over a predetermined length l_1 of the base pin 1, remote from the primary fixation element 2 (which has a length l_3). The mutual distance between the first and secondary fixation elements 2, 6 can thus be selected dependent on the specific situation.

[0022] Furthermore, the connection part 3 comprises a plurality of restrictions 11 (e.g. in the form of indentations, or a stepped or sinusoid cylinder profile) having an outer diameter d_1 different from a local outer diameter d_2 of the base pin 1, indicated by surface 10. This is shown in detail in the enlarged partial view of the connection part in Fig. 2. In the embodiment shown, the outer diameter d_1 is smaller (e.g. 1.3mm) than the local outer diameter d_2 (e.g. 2 mm), which can e.g. be accomplished by a simple milling process step of the base pin 1.

[0023] An embodiment of the secondary fixation element 6 is shown in more detail in a side view in Fig. 4a and in a cross sectional view in Fig. 4b. In order to be able to shift or slide the secondary fixation element 6 over the handling part 4 and the connection part 3, the secondary fixation element 6 has a bore with an inner diameter which is larger than an outer diameter of the base pin 1 in a further embodiment (e.g. 2.2mm and 2.0mm).

[0024] In a further embodiment, the secondary fixation element 6 comprises a self tapping (and intra-cortical) threaded part 12, allowing to fixate the secondary fixation element 6 to the other part of the (fractured) clavicle. The size and pitch of the threaded part 12 may be 25 similar to the size and pitch of the threaded head end 2a of the primary fixation element 2. As shown most clearly in the side view of Fig. 3a, the secondary fixation element 6 is provided with a plurality of slots 15 in the self-tapping threaded part 12. These slots 15 allow fixation of the secondary fixation element 6 using a special tool sliding over entire exposed part of the base pin 1, as will be discussed in more detail below.

[0025] To ascertain that the primary and secondary fixation elements 2, 6 stay at the set distance from each other, the secondary fixation element 6 comprises a locking end 17 having a plurality of resilient legs 14 each having an inwardly extending end part 16 in a further embodiment. The resilient legs 14 press the inwardly extending parts 16 into the restrictions 11 of the connection part 3, thereby fixing the set distance, yet allowing rotation. Alternatives would e.g. be to use another pressure exerting element, e.g. one or more leaf springs, etc.

[0026] To lock the secondary element 6 into position with respect to the connection part 3, in a further embodiment the locking end 17 is provided with an outer thread and the secondary fixation element 6 further comprises a locking screw 7 as implementation of the end cap 7. A perspective view of the locking screw is shown in Fig. 4a, and a cross sectional view in Fig. 4b. The locking

screw 7 is provided with an internal screw thread 7b matching the external screw thread on the resilient legs 14, and furthermore comprises a slit 7a allowing a screw driver type of installation of the locking screw 7.

[0027] In a further aspect, the present invention also relates to a kit for a fracture of a long pipe bone, such as a clavicle fracture, comprising an intramedullary device according to any one of the embodiments as described above. Furthermore, the kit comprises a first tool for fixing the primary fixation element 2 of the base pin 1 in a medial part of the long pipe bone/ clavicle (e.g. using a handle bar attached to the handling part 4), and a second tool 8 for fixing the secondary fixation element 6 to a further part of the long pipe bone/clavicle. An embodiment of this second tool is shown in the perspective view of Fig. 5, and is e.g. shaped as a hollow cylinder, able to slide over the still remaining parts of the base pin 1. The second tool 8 is provided with extending parts 8a, matching the slots 15 on the secondary fixation element 6, and allowing to exert sufficient torque to properly fixate the secondary fixation element 2 in the clavicle.

[0028] Once the secondary fixation element 6 is secured in the long pipe bone/ clavicle, the base pin 1 can be cut to length (e.g. at one of the restrictions 11 of the connection part 3), e.g. using a generally available (surgical) cutting tool, or a specific cutting tool being part of the kit. After that, the locking screw 7 can be positioned over the resilient legs 14 of the secondary fixation element, and fastened using a third tool 9 for attaching the secondary fixation element 6 to the connection part 3 of the base pin 1. The third tool is shown in perspective in Fig. 6 and is provided with a first end having a screwdriver type (flat) head 9a, matching the slit 7a of the locking screw 7. Furthermore, the third tool 9 may be provided with a handling part 9b, similar to the handling part 4 of the base pin 1, allowing e.g. to attach a handle to allow a screwing motion of the third tool 9.

[0029] In summary, the innovative aspect of the device developed lies in being an intramedullary device that is able to re-establish anatomical alignment, prevent shortening and its ability to rotate freely within itself. Especially the latter is the key to the new intramedullary device for MSCF, but also very usable for treatment of other fractures involving long pipe bones. This should be made possible by its design as summarized above and as shown in the drawing embodiments.

[0030] The present invention embodiments have been described above with reference to a number of exemplary embodiments as shown in the drawings. Modifications and alternative implementations of some parts or elements are possible, and are included in the scope of protection as defined in the appended claims.

55 Claims

1. Intramedullary device for treatment of a fracture of a long pipe bone, comprising

- a base pin (1) having a primary fixation element (2) and a connection part (3),
 - a secondary fixation element (6) attachable to the connection part (3) at one of a plurality of predetermined distances along the base pin with respect to the primary fixation element (2),
characterised in that: the secondary fixation element (6) has a bore with an inner diameter which is larger than an outer diameter of the base pin so that the secondary fixation element (6) can be slid or shifted over the connection part (3), and **in that:** the secondary fixation element comprises a locking end for preventing axial movement of the first fixation element relative to the second fixation element when attached, whilst allowing the connection part (3) of the base pin (1) and the secondary fixation element (6) to rotate with respect to each other.
2. Intramedullary device according to claim 1, wherein the connection part (3) is provided over a predetermined length (l_1) of the base pin (1).
 3. Intramedullary device according to claim 1 or 2, wherein the connection part (3) comprises a plurality of restrictions (11) having an outer diameter (d_1) different from a local outer diameter (d_2) of the base pin (1).
 4. Intramedullary device according to any one of claims 1-3, wherein the secondary fixation element (6) has a bore with an inner diameter which is larger than an outer diameter of the base pin (1).
 5. Intramedullary device according to any one of claims 1-4, wherein the locking end (17) has a plurality of resilient legs (14) each having an inwardly extending end part (16).
 6. Intramedullary device according to claim 5, wherein the locking end (17) is provided with an outer thread and the secondary fixation element (6) further comprises an end cap (7).
 7. Intramedullary device according to any one of claims 1-6, wherein the secondary fixation element (6) comprises a self-tapping threaded part (12).
 8. Intramedullary device according to claim 7, wherein the secondary fixation element (6) is provided with a plurality of slots (15) in the self-tapping threaded part (12).
 9. Intramedullary device according to any one of claims 1-8, wherein the primary fixation element (2) comprises a self-tapping threaded head end (2a).
 10. Intramedullary device according to claim 9, wherein the self-tapping threaded head end (2a) is provided with a blunt tip part (2b).
 11. Intramedullary device according to any one of claims 1-10, wherein the base pin (1) further comprises a handling part (4) remote from the primary fixation element (2).
 12. Intramedullary device according to any one of claims 1-11, wherein the base pin (1) is bendable.
 13. Kit for a fracture of a long pipe bone, such as a clavicle fracture, comprising an intramedullary device according to any one of claims 1-12,
 - a first tool for fixing the primary fixation element (2) of the base pin (1) in a medial part of the long pipe bone,
 - a second tool (8) for fixing the secondary fixation element (6) to a further part of the long pipe bone, and
 - a third tool (9) for attaching the secondary fixation element (6) to the connection part (3) of the base pin (1).
 14. Kit according to claim 13, further comprising a cutting tool for cutting the connection part (3) to a final length of the base pin (1).

Patentansprüche

1. Intramedulläre Vorrichtung zur Behandlung einer Fraktur eines langen Röhrenknochens, umfassend
 - einen Basisstift (1) mit einem primären Fixierungselement (2) und einem Verbindungsteil (3),
 - ein sekundäres Fixierungselement (6), das in einem von einer Vielzahl von vorbestimmten Abständen entlang des Basisstifts in Bezug auf das primäre Fixierungselement (2) an dem Verbindungsteil (3) befestigt werden kann,

dadurch gekennzeichnet, dass das sekundäre Fixierungselement (6) eine Bohrung mit einem Innendurchmesser, der größer ist als ein Außendurchmesser des Basisstifts, aufweist, so dass das sekundäre Fixierungselement (6) über den Verbindungsteil (3) gezogen oder geschoben werden kann, und dass das sekundäre Fixierungselement ein Verriegelungsende umfasst, um eine axiale Bewegung des ersten Fixierungselements relativ zu dem zweiten Fixierungselement, wenn es befestigt ist, zu verhindern, während der Verbindungsteil (3) des Basisstifts (1) und das sekundäre Fixierungselement

- (6) gegeneinander rotieren können.
2. Intramedulläre Vorrichtung gemäß Anspruch 1, wobei der Verbindungsteil (3) über eine vorbestimmte Länge (l_1) des Basisstifts (1) vorhanden ist. 5
 3. Intramedulläre Vorrichtung gemäß Anspruch 1 oder 2, wobei der Verbindungsteil (3) eine Vielzahl von Restriktionen (11) umfasst, die einen Außendurchmesser (d_1) aufweisen, der von einem lokalen Außendurchmesser (d_2) des Basisstifts (1) verschieden ist. 10
 4. Intramedulläre Vorrichtung gemäß einem der Ansprüche 1 bis 3, wobei das sekundäre Fixierungselement (6) eine Bohrung mit einem Innendurchmesser, der größer ist als ein Außendurchmesser des Basisstifts (1), aufweist. 15
 5. Intramedulläre Vorrichtung gemäß einem der Ansprüche 1 bis 4, wobei das Verriegelungsende (17) eine Vielzahl von elastischen Beinen (14) aufweist, die jeweils einen sich nach innen erstreckenden Endteil (16) aufweisen. 20
 6. Intramedulläre Vorrichtung gemäß Anspruch 5, wobei das Verriegelungsende (17) mit einem Außengewinde versehen ist und das sekundäre Fixierungselement (6) weiterhin eine Endkappe (7) umfasst. 25
 7. Intramedulläre Vorrichtung gemäß einem der Ansprüche 1 bis 6, wobei das sekundäre Fixierungselement (6) einen selbstschneidenden Gewindeteil (12) umfasst. 30
 8. Intramedulläre Vorrichtung gemäß Anspruch 7, wobei das sekundäre Fixierungselement (6) mit einer Vielzahl von Schlitzten (15) in dem selbstschneidenden Gewindeteil (12) versehen ist. 35
 9. Intramedulläre Vorrichtung gemäß einem der Ansprüche 1 bis 8, wobei das primäre Fixierungselement (2) ein mit einem selbstschneidenden Gewinde versehenes Kopfende (2a) umfasst. 40
 10. Intramedulläre Vorrichtung gemäß Anspruch 9, wobei das mit einem selbstschneidenden Gewinde versehene Kopfende (2a) mit einem stumpfen Spitzenteil (2b) versehen ist. 45
 11. Intramedulläre Vorrichtung gemäß einem der Ansprüche 1 bis 10, wobei der Basisstift (1) weiterhin einen vom primären Fixierungselement (2) entfernt liegenden Handhabungsteil (4) umfasst. 50
 12. Intramedulläre Vorrichtung gemäß einem der Ansprüche 1 bis 11, wobei der Basisstift (1) biegsam ist. 55

13. Kit für eine Fraktur eines langen Röhrenknochens, wie eine Schlüsselbeinfraktur, umfassend eine intramedulläre Vorrichtung gemäß einem der Ansprüche 1 bis 12, ein erstes Werkzeug zum Fixieren des primären Fixierungselements (2) des Basisstifts (1) in einem medialen Teil des langen Röhrenknochens, ein zweites Werkzeug (8) zum Fixieren des sekundären Fixierungselements (6) an einem weiteren Teil des langen Röhrenknochens und ein drittes Werkzeug (9) zum Befestigen des sekundären Fixierungselements (6) an dem Verbindungsteil (3) des Basisstifts (1).
14. Kit gemäß Anspruch 13, weiterhin umfassend ein Schneidwerkzeug zum Schneiden des Verbindungsteils (3) auf eine endgültige Länge des Basisstifts (1).

Revendications

1. Dispositif intramédullaire pour le traitement d'une fracture d'un os long, comprenant
 - une broche de base (1) comportant un élément de fixation primaire (2) et une partie de connexion (3),
 - un élément de fixation secondaire (6) pouvant être fixé (3) à l'une d'une pluralité de distances prédéterminées disposées le long de la broche de base par rapport à l'élément de fixation primaire (2) de la partie de connexion

caractérisé en ce que: l'élément de fixation secondaire (6) présente un alésage d'un diamètre intérieur supérieur à un diamètre extérieur de la broche de base de sorte que l'élément de fixation secondaire (6) puisse être glissé ou décalé au-dessus de la partie de connexion (3),
et en ce que: l'élément de fixation secondaire comprend une extrémité de verrouillage pour empêcher le mouvement axial du premier élément de fixation par rapport au deuxième élément de fixation une fois fixé, tout en permettant à la partie de connexion (3) de la broche de base (1) et l'élément de fixation secondaire (6) de tourner l'un par rapport à l'autre.
2. Dispositif intramédullaire selon la revendication 1, dans lequel la partie de connexion (3) est présente sur une longueur prédéterminée (l_1) de la broche de base (1).
3. Dispositif intramédullaire selon la revendication 1 ou 2, dans lequel la partie de connexion (3) comprend une pluralité de zones en retrait (11) ayant un diamètre extérieur (d_1) différent d'un diamètre extérieur

- local (d_2) de la broche de base (1).
4. Dispositif intramédullaire selon l'une quelconque des revendications 1 à 3, dans lequel l'élément de fixation secondaire (6) présente un alésage dont le diamètre interne est supérieur au diamètre externe de la broche de base (1).
- 5 14. Kit selon la revendication 13, comprenant en outre un outil de coupe pour couper la partie de connexion (3) à une longueur finale de la broche de base (1).
5. Dispositif intramédullaire selon l'une quelconque des revendications 1 à 4, dans lequel l'extrémité de verrouillage (17) comporte une pluralité de pattes élastiques (14) ayant chacune une partie d'extrémité s'étendant vers l'intérieur (16).
- 10
6. Dispositif intramédullaire selon la revendication 5, dans lequel l'extrémité de verrouillage (17) est munie d'un filetage extérieur et l'élément de fixation secondaire (6) comprend en outre un capuchon d'extrémité (7).
- 15
7. Dispositif intramédullaire selon l'une quelconque des revendications 1 à 6, dans lequel l'élément de fixation secondaire (6) comprend une partie filetée auto-taroudante (12).
- 20
8. Dispositif intramédullaire selon la revendication 7, dans lequel l'élément de fixation secondaire (6) est pourvu d'une pluralité de fentes (15) dans la partie filetée auto-taroudante (12).
- 25
9. Dispositif intramédullaire selon l'une quelconque des revendications 1 à 8, dans lequel l'élément de fixation primaire (2) comprend une extrémité en tête filetée auto-taroudante (2a).
- 30
10. Dispositif intramédullaire selon la revendication 9, dans lequel l'extrémité en tête filetée auto-taroudante (2a) est munie d'une partie en pointe émoussée (2b).
- 35
11. Dispositif intramédullaire selon l'une quelconque des revendications 1 à 10, dans lequel la broche de base (1) comprend en outre une partie de manipulation (4) distante de l'élément de fixation primaire (2).
- 40
12. Dispositif intramédullaire selon l'une quelconque des revendications 1 à 11, dans lequel la broche de base (1) est flexible.
- 45
13. Kit pour fracture d'un os long, tel qu'une fracture de clavicule, comprenant un dispositif intramédullaire selon l'une quelconque des revendications 1 à 12, un premier outil pour fixer l'élément de fixation primaire (2) de la broche de base (1). dans une partie médiane de l'os long, un deuxième outil (8) pour fixer l'élément de fixation secondaire (6) en une autre partie de l'os long et
- 50
- 55

Fig. 1

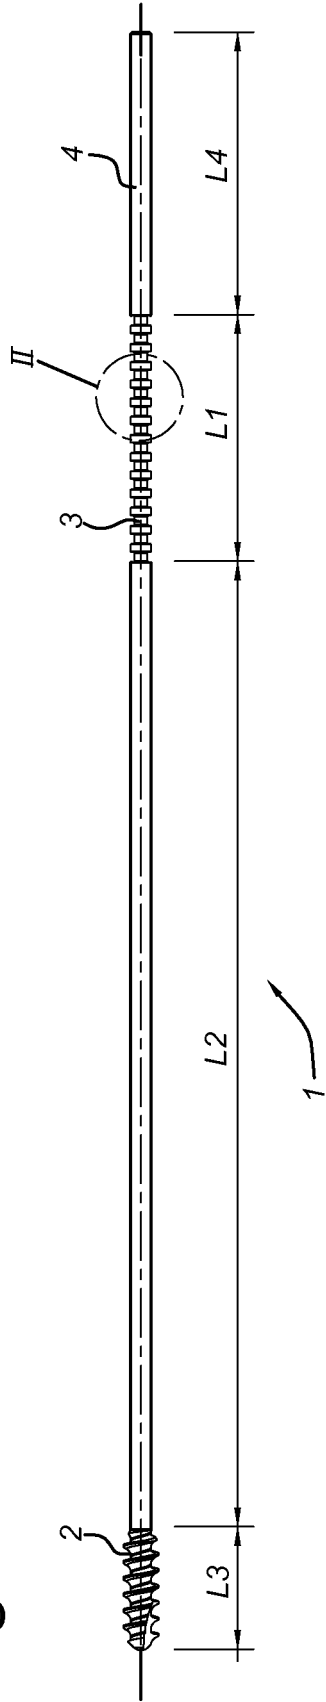


Fig. 2

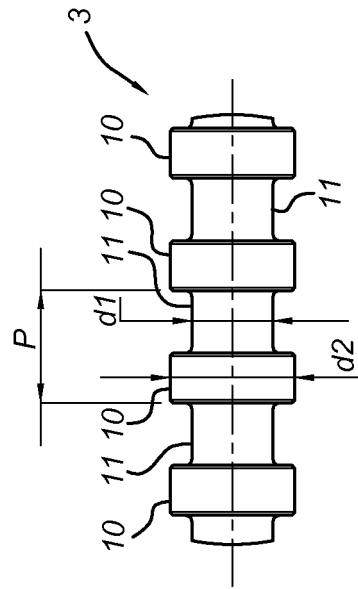


Fig. 3a

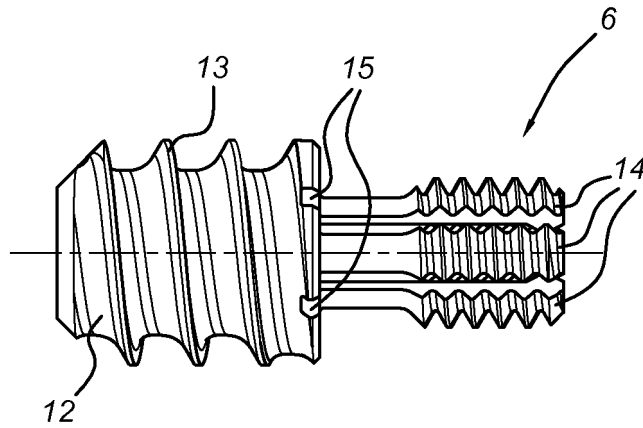


Fig. 3b

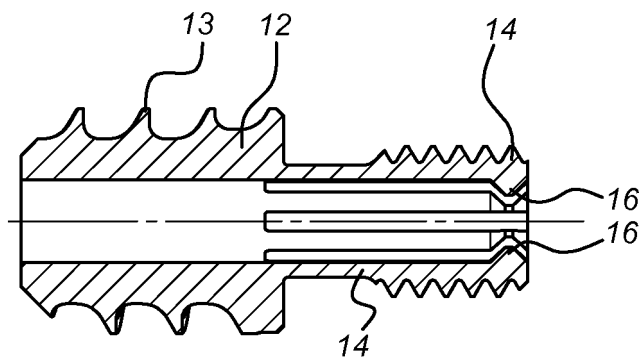


Fig. 4a

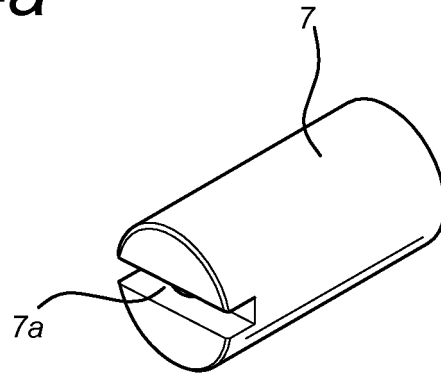


Fig. 4b

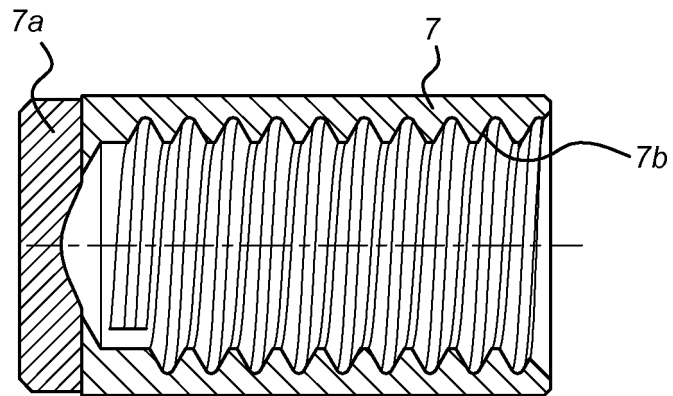


Fig. 5


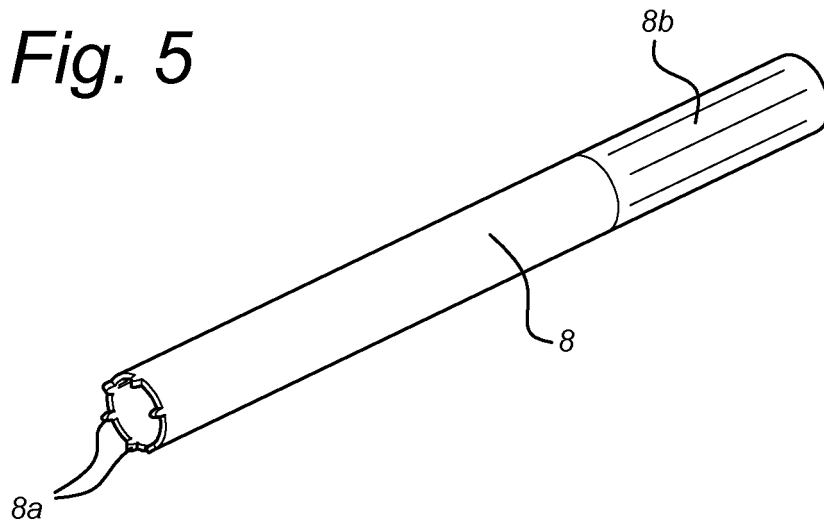


Fig. 6

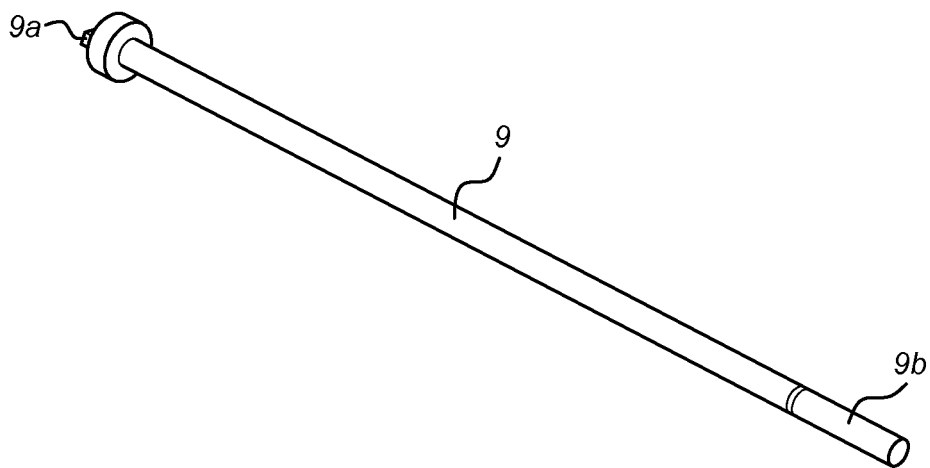

REFERENCES CITED IN THE DESCRIPTION

This list of references cited by the applicant is for the reader's convenience only. It does not form part of the European patent document. Even though great care has been taken in compiling the references, errors or omissions cannot be excluded and the EPO disclaims all liability in this regard.

Patent documents cited in the description

- US 4640271 A [0002]
- US 2009306718 A [0003]
- US 6338732 B [0004]
- US 20110009865 A [0005]
- WO 2011060412 A [0006]
- US 5374235 A [0007]